




ASTM C 1202-97



Test-compagny
Testing street 45
CompagnyCity
Some Country

Your own logo.
size=20x80mm




GERMANN INSTRUMENTS

DENMARK
Phone: +45 3967 7117
Fax: +45 3967 3167

USA
Phone: (847)329-9999
Fax: (847)329-8888

Test report

Voltage Used: 60
 Testing time: 06:00 hour
 Charge passed: 3947
 Adjusted Charge passed: 3562
 Permeability class: Moderate
 Instrument number: 072707
 Channel number: 2
 Report date: 25/04/2014
 Testing by: ---
 Reference: ---
 Sample diameter: 100
 Comment: ---

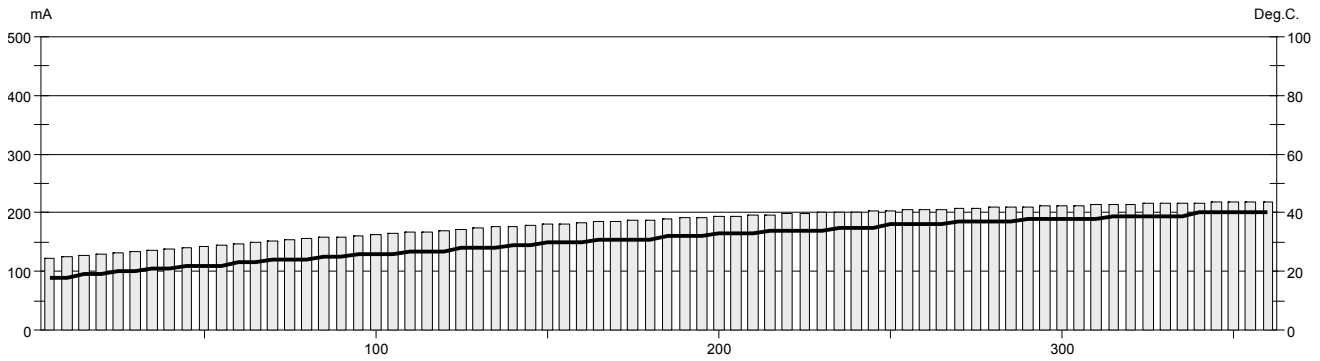

Time	°C	mA	Time	°C	mA	Time	°C	mA	Time	°C	mA
00:05	18	123.4	01:35	26	161.3	03:05	32	189.9	04:35	37	207.9
00:10	18	125.7	01:40	26	163.2	03:10	32	191.2	04:40	37	208.8
00:15	19	128.0	01:45	26	164.9	03:15	32	192.4	04:45	37	209.7
00:20	19	130.2	01:50	27	166.8	03:20	33	193.6	04:50	38	210.2
00:25	20	132.4	01:55	27	168.5	03:25	33	194.9	04:55	38	211.1
00:30	20	134.5	02:00	27	170.1	03:30	33	196.1	05:00	38	211.8
00:35	21	136.8	02:05	28	171.9	03:35	34	196.9	05:05	38	212.6
00:40	21	139.1	02:10	28	173.7	03:40	34	198.0	05:10	38	213.6
00:45	22	141.1	02:15	28	175.3	03:45	34	198.9	05:15	39	214.3
00:50	22	143.3	02:20	29	176.9	03:50	34	199.8	05:20	39	215.0
00:55	22	145.4	02:25	29	178.2	03:55	35	200.9	05:25	39	215.5
01:00	23	147.6	02:30	30	180.0	04:00	35	201.9	05:30	39	216.1
01:05	23	149.6	02:35	30	181.5	04:05	35	202.9	05:35	39	216.6
01:10	24	151.6	02:40	30	183.0	04:10	36	203.6	05:40	40	217.3
01:15	24	153.5	02:45	31	184.4	04:15	36	204.4	05:45	40	217.9
01:20	24	155.6	02:50	31	185.8	04:20	36	205.3	05:50	40	218.5
01:25	25	157.5	02:55	31	187.1	04:25	36	206.1	05:55	40	218.9
01:30	25	159.4	03:00	31	188.5	04:30	37	207.2	06:00	40	219.3